


SCALE 0.500

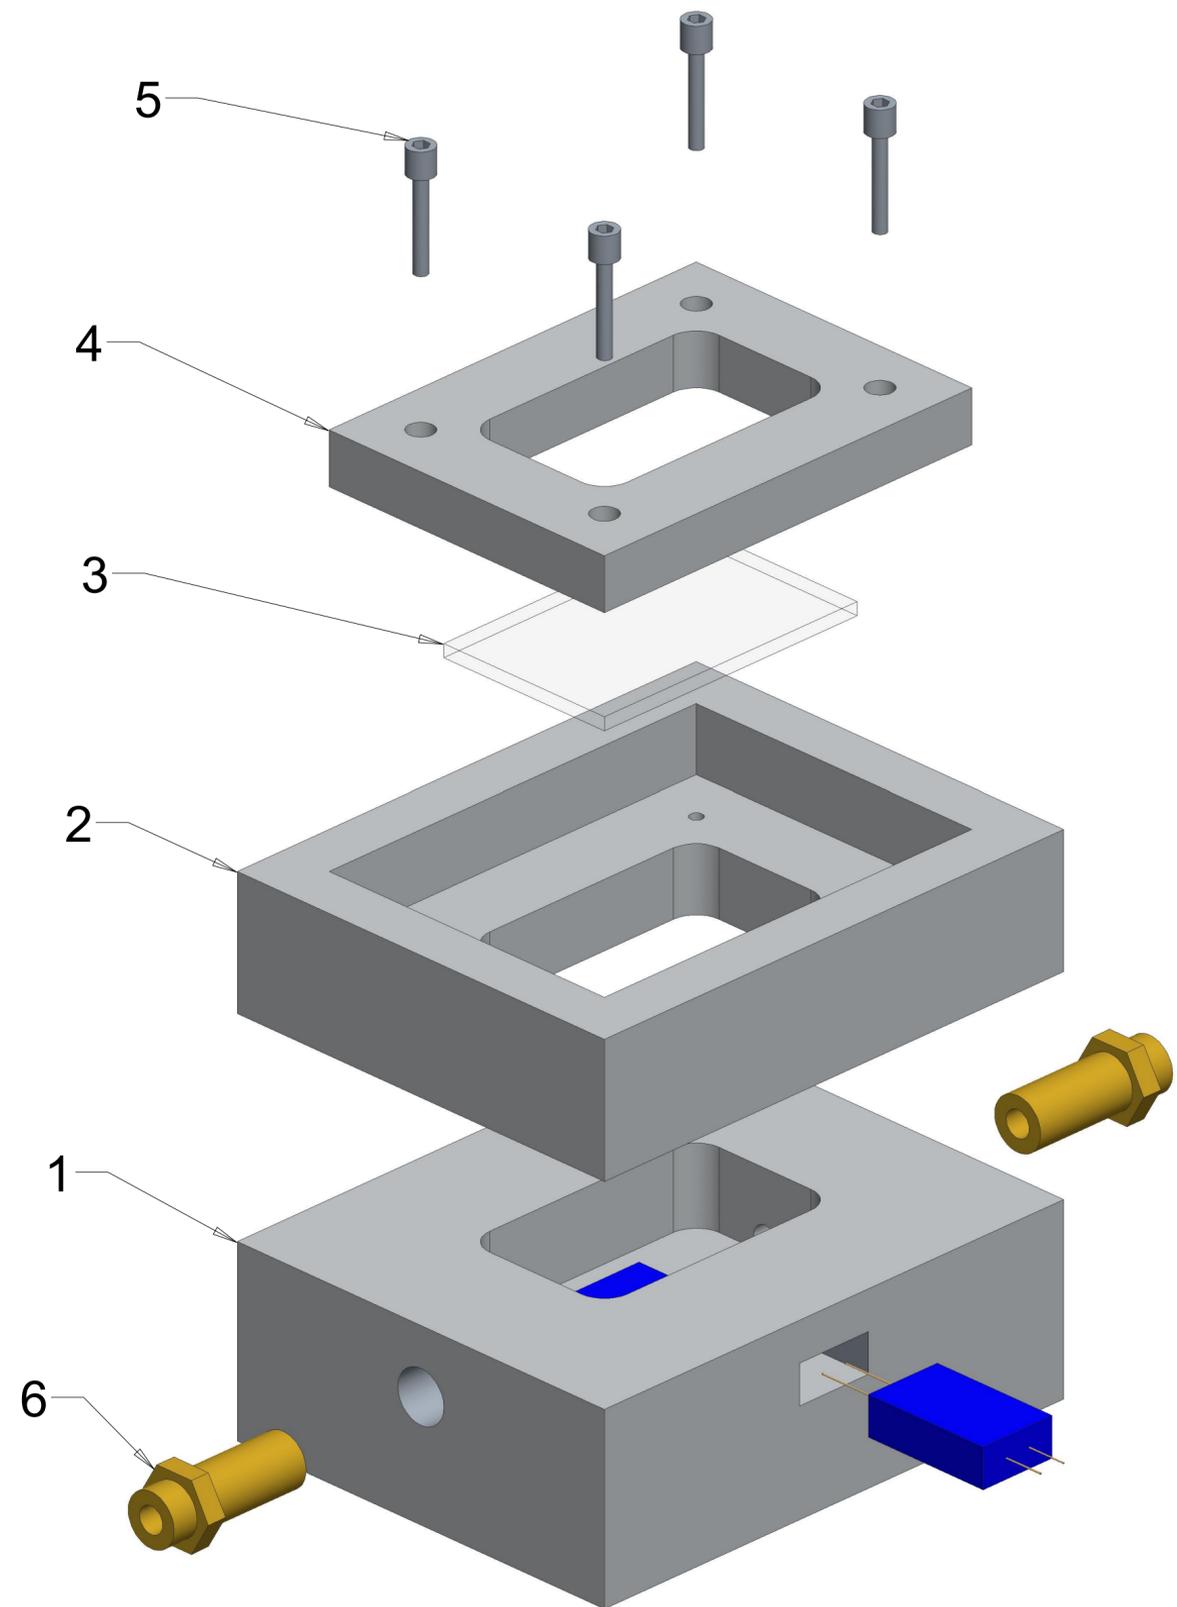

SCALE 0.500

PART NUMBER	PART NAME	QUANTITY	NOTES
1	BASE	1	INSULATING MATERIAL (CERAMIC) AND GOLD WIRES TO BE INSTALLED AFTER BASE IS CONSTRUCTED.
2	HATCH	1	HATCH WILL TO BE ATTACHED TO LID WITH (2) SMALL HINGES AND (2) SMALL LATCHES ON OPPOSITE SIDES.
3	WINDOW	1	WINDOW TO BE HELD IN PLACE BY SCREWS. TO BE MADE WITH TRANSPARENT MATERIAL (HYPOXY, GLASS, ETC.).
4	LID	1	LID TO BE INSTALLED ON TOP OF WINDOW. HELD IN PLACE BY SOCKET CAP SCREWS (SAME AS EXISTING).
5	SCREWS	4	SOCKET CAP SCREWS TO BE INSTALLED. DIAMETER MAY BE BETWEEN 0.15 CM AND 0.5 CM. MUST BE AT LEAST 1.5 CM LENGTH.
6	NOZZLE	2	NOZZLE SIMILAR TO EXISTING GAS CHAMBER TO BE USED. MUST CONNECT TO THE GAS INFLOW PIPE.